


A. C. CONSTANTS

f	C ₁	C ₂	C ₃	C ₄	C ₅	C ₆	R ₁	R ₂	R ₃
60~	0.7	0.08	0.015	0.015	0.006	0.002	11	98	96.0
50~	0.84	0.096	0.018	0.018	0.0072	0.0024	13.2	118	115.2
42~	1.0	0.114	0.021	0.021	0.0086	0.0029	15.7	140	137.1
30~	1.4	0.16	0.03	0.03	0.012	0.004	2.2	196	192.0
25~	1.68	0.192	0.036	0.036	0.0144	0.0048	26.4	235	230.4

Condensers C₁, C₂, C₃, C₄, C₅, C₆ calibrated to individual instruments.

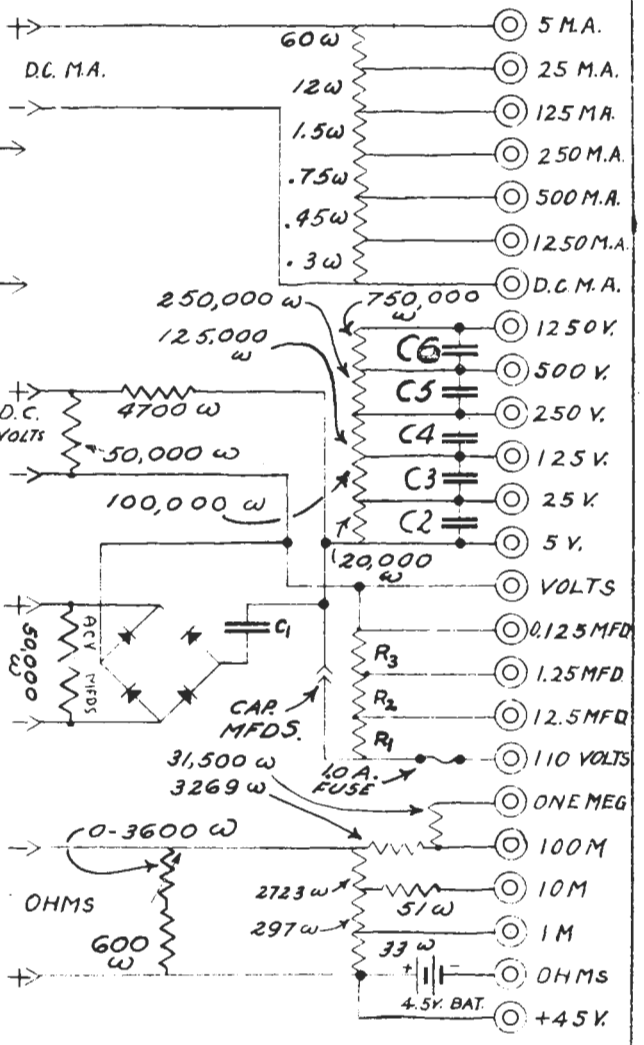

Revised: 6-30-33
 Revised & retraced: 8-12-33
 Revised - 11-11-33 - Capacity Switch
 Identified in terms of Panel
 markings. Revised - 11-17-33
 Revised - 3/12-54.

DRAWN - TRACED
 CHECKED
 APPROVED

SUPREME INSTRUMENTS CORP.
 GREENWOOD - MISS.
 5-12-33

SCHEMATIC WIRING DIAGRAM
 MODEL 333
 707A



www.StevenJohnson.com

**Antique Technolgy, Tube Radios and Test Equipment
Vintage Schematics, and Publications**

Steve's Antique Technology